

STEP 1 - APRIL '23

Serial No. C 103218

Weightron Bilanciai Ltd,
Titan Works
Bridge Way off Broombank Road,
Chesterfield Trading Estate,
Chesterfield S41 9QJ, UK
Tel: 01246 260062
Fax: 01246 260844
www.weightron.com



Weightron Bilanciai Ltd,
Unit 4b, Block 4
Westpark, Chelston
Wellington TA21 9AD, UK
Tel: 01823 662355
Fax: 01823 662017
www.weightron.com



CALIBRATION CERTIFICATE

This Calibration Certificate is issued in accordance with the UKWF Code of Practice for the calibration of Non Automatic Weighing Machines. All weights used are traceable to NPL

Customer

ENVIRONCOM LTD SPIFFLEGATE LEVEL GRANTHAM NG31 7UH LOCATION

Machine Details

Cust ref	STEP 1
Make	NEWTON
Model	NT-201A
Ser No	030900162
Capacity	2000 / kg
e/d	/ / kg
Working cap	

Test Weights

Set No.	Cert No.	Date Cal
5	09862	09/01/23

Cert Interval	ANNUALLY
Next Cert	APR 2024


Tolerance +/-	kg
0- 1000	1
1000-2000	2

Comments MAKE UP WEIGHT USED 932 kg	<table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="padding: 5px; width: 50px; height: 50px; text-align: center;">2</td> <td style="padding: 5px; width: 50px; height: 50px; text-align: center;">3</td> </tr> <tr> <td style="padding: 5px; height: 50px; text-align: center;">1</td> <td style="padding: 5px; height: 50px; text-align: center;">4</td> </tr> </table> *	2	3	1	4
2	3				
1	4				

AS FOUND LINEARITY & HYSTERESIS

Load	Loading	Dev	Unloading	Dev
0	0	0	0	0
60	60	0	60	0
100	100	0	100	0
140	140	0	140	0
200	200	0	200	0
932	932	0	932	0
1132	1132	0	1132	0


DEFINITIVE LINEARITY & HYSTERESIS

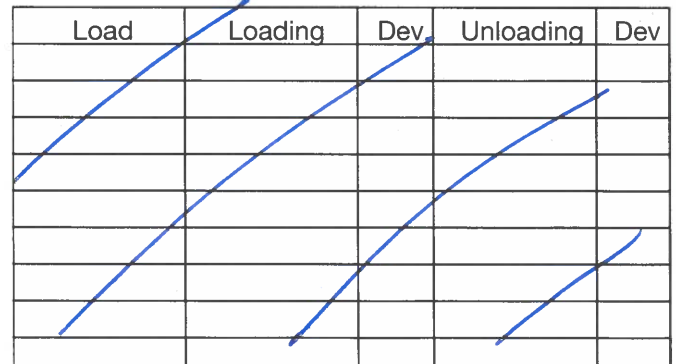

Repeatability 932

Load	Ind	Ind	Ind
932	932	932	/


Repeatability

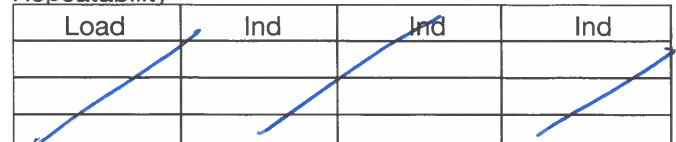

Eccentric Load 200

Reading	Dev	Reading	Dev
1 200	0	2 200	0
3 200	0	4 200	0
5		6	
7		8	

Eccentric Load

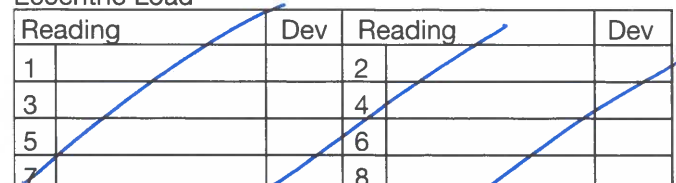

Signature *[Signature]* Name D. PEAKE Date 05/04/2023